



ErsaTec

process - analyzers

Hydrocarbon Analyzer SmartFID ST

ErsaTec GmbH

Dahlkampsanger 5
D-30890 Barsinghausen

Tel.: +49 5105 520558

Fax: +49 5105 529184

www.ersatec.com
info@ersatec.com



// Our fix SmartFID system


The SmartFID ST is the fix installed 19" version of our SmartFID. This device also brings our FID-principle and the SPS-technology together. And the handling is very easy, too.

Properties:

- large display
- Touch-Screen handling
- Ethernet connection
- fires up automatically
- heats up automatically
- automatic fuel gas switch of
- automatic change of measuring range
- 19" device for installation in a fix measuring
- diverse and comfortable opportunities to configure.
for example alarm limits, logging interval ...

Advantages:

- 19" design (4 RU)
- automatic operation with
extensive self-operated
monitoring and securityfunctions
- internal datalogging
- network-compatible
- approved detector-geometry
- low fuel gas consumption
- low operating cost
- internal temperature control for
heated pipes

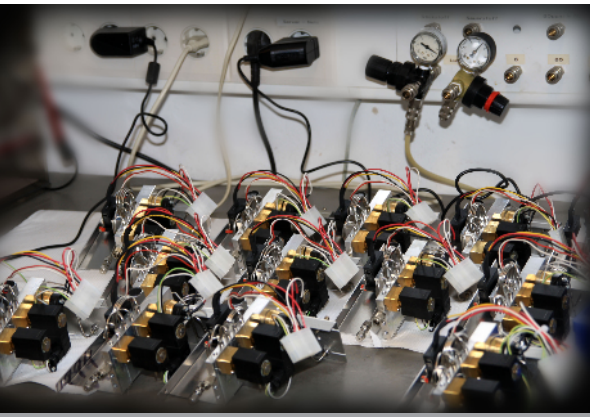

measuring components	hydrocarbons, chlorinated hydrocarbons
measuring principle	flame-ionization-detection (FID)
measuring ranges (relative to C ₃ H ₈)	5 selectable ranges/ automatic measuring range change-over: standard: 0 ... 10 ppm bis 0 ... 10 Vol.% optionale probe measuring ranges: 0 ... 1 ppm bis 0 ... 1 Vol.%, additionally free configurable measuring ranges
detection limit	≤1,5% of upper range value
linearity	±1,0% of selected range
repeatability	≤1,0% at constant temperature and constant pressure
zero-point-drift	≤0,5% of upper range value per month
sensitivity-drift	≤2,8% of upper range value per week
O ₂ -cross-sensitivity	<4% related to 8 ppm C ₃ H ₈
warm-up time	25 min
T ₉₀ -time	typ. 20 s
measuring gas conditions	
pressure	atmospheric ±0,05 bar
temperature	0-230 °C
flow	approx. 1,2 l/min
sample gas connection	clamp collar screwing for stainless steel tube, OD 6 mm
supporting gases	
fuel gas	hydrogen, category 5.0, residual content of hydrocarbons <0,5 ppm, pressure: 3 bar, consumption in continuous operation: 1,2 l/h; alternatively H ₂ /He-mixture, consumption: approx. 2,4 l/h
calibration gas	concentration of approx. 80% of range (typ. propane) in synthetic air, pressure: 3 bar, consumption during calibration process: 1,6 l/min
combustion air/ zero gas	air quality class 1.2.1 at the extraction point according to DIN 2010
connector	quick coupling
energy supply	115 or 230 V AC 48 ... 63 Hz; power consumption: maximal 350 W on heating process typ. 120 W during operation
weight	analyser: 9 kg
dimensions (H x W x D)	177 mm (4 RU) x 445 mm (19") x 365 mm
signal outputs	
analog outputs	2 free configurable 0...4 - 20 mA outputs
digital outputs	3 free configurable potential-free contacts, 250 V AC 1 A
conformities	CE, EMV, VDE 0701



Fields Of Application:


SmartFID is suitable for measurement of

- emissions from thermic, catalytic, biological, and activated charcoal exhaust air purification plants
- maximum work place concentration value
- hydrocarbon emission in crude gas and clean gas
- process monitoring and control of manufacturing plants
- emissions from (combustion) engines
- detection of hydrocarbon breakthroughs in exhaust air purifiers and chemical cleaning plants
- emissions on power plants, garbage incineration plants and mechanical waste treatment plants


// SmartFID Measuring Principle

Flame Ionisation Detectors (FID) are known to be reliable and robust analysers in the domain of volatile organic compounds (VOC) analysis..

In the measurement process the gas sample is continuously taken into the FID via a heated sample drawing. There the gas sample is burned up in a hydrogen diffusion flame. If the sample gas contains VOC the organic compounds will be cracked up in the combustion process when getting into the flame. This produces CH fragments that react with atomic oxygen so that CHO ions are generated. These ions are stripped in an electric field and a small electrical current is generated which is proportional to the amount of fed VOCs.

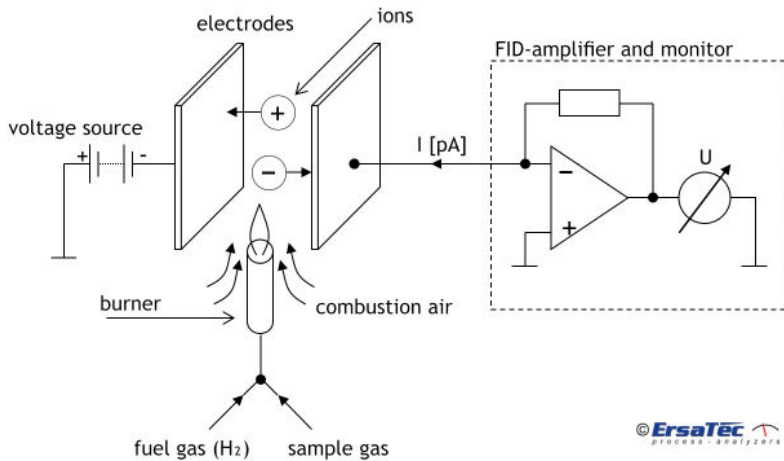

© ErsaTec
PROCESS - ANALYZERS

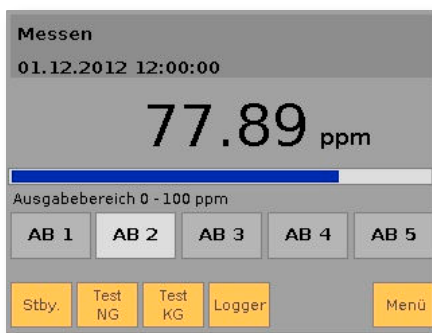

For more information: www.ersatec.com

About Us:

ErsaTec is your reliable service partner in terms of analysing dangerous hydrocarbon with the FID measuring principle. We offer you our complete service, including to check your SmartFID devices. Also you'll find all the information you'll need about our modern products.

If you have problems with your product or need our help in general, just contact us!